



# LIFEPAK® CR2 Defibrillator with LIFELINKcentral™ AED Program Manager

## Getting Started Guide

1





## Indications for Use

The LIFEPAK CR2 defibrillator is indicated for use on patients 1 year of age or older in cardiopulmonary arrest. The patient must be unresponsive (unconscious), not breathing normally, and showing no signs of circulation (for example, no pulse, no coughing, or no movement).

The cprCOACH™ Feedback Technology in the LIFEPAK CR2 defibrillator is indicated for use on cardiopulmonary arrest patients and provides CPR guidance in accordance with the AHA Guidelines for patients 1 year of age or older.

The LIFEPAK CR2 defibrillator is intended for use by personnel who have been trained in its operation. Users should have received training in basic life support/ AED, advanced life support, or a physician-authorized emergency medical response training program.

The LIFEPAK CR2 defibrillator is indicated to be used with the QUIK-STEP™ pacing/ECG/defibrillation electrodes and the LIFEPAK CR2 lithium battery.

## Contraindications

The LIFEPAK CR2 defibrillator is not indicated for patients who are conscious and responsive.

For information regarding the LIFEPAK CR2 defibrillator Clinical Summaries and Potential Adverse Effects, see the *LIFEPAK CR2 Defibrillator Operating Instructions*.

## Important Information

!USA Rx Only

---

---

**LIFEPAK® CR2** Defibrillator  
with **LIFELINKcentral™** AED Program Manager

Thank you for making defibrillation readily available to your workplace or community so that, when a heart stops beating, lifesaving treatment is just minutes away.

Please ensure the LIFEPAK CR2 Defibrillator is 'Connected and Ready' for use in an emergency by following these simple instructions.

## Defibrillator Management

Physio-Control offers web-based services that can monitor your LIFEPAK CR2 defibrillator (AED) and ensure it is ready for use. These services are LIFELINKcentral AED Program Manager and LIFENET® System.

**LIFELINKcentral AED Program Manager** is used by customers to manage AEDs.

**LIFENET System** is used by health care organizations that have additional emergency equipment.

**Note:** LIFELINKcentral AED Program Manager and LIFENET System are not available in all countries.

## The Connected AED

If your LIFEPAK CR2 defibrillator has wireless capability, it can connect to the internet and report its status to LIFELINKcentral AED Program Manager or LIFENET System. If the AED is not ready or fails to check in, an email notification is sent to your organization's account administrator. Email notifications are also sent if a battery or electrode expiration date is approaching.

**Note:** The AED does not have to be connected to function. You can verify the AED is ready for use by checking the Readiness indicator as described in step 6 of this guide.

---

---

## How the AED Connects

The AED can connect to LIFELINKcentral AED Program Manager or LIFENET System using a Wi-Fi®, cellular, or USB connection to the internet.

### LIFEPAK CR2 Defibrillator Connectivity



**Note:** The micro-USB port is to be used by authorized users only. The micro-USB port does not provide power and should not be connected to other devices, such as mobile phones or other USB connected products.

---

---

# 1

## Unpack the LIFEPAK CR2 defibrillator (AED)

Take contents out of the box and check them against the sales order.

If something is missing from the shipping box, please call Physio-Control Customer Support or your local authorized distributor as soon as possible. See the contact list included in the box for region-specific phone numbers.

---

# 2

## Confirm the Date of Manufacture on the battery


The date of manufacture is printed on the battery label in YYYY-MM-DD format. The battery must be installed within 1 year of this date. For detailed information about battery service life, see the *LIFEPAK CR2 Defibrillator Operating Instructions*.



# 3

Determine if the AED has Wi-Fi® or cellular capability.

All LIFEPAK CR2 defibrillators have USB capability. To determine if the AED also has wireless (Wi-Fi or Cellular) capability, check the serial number label located in the battery compartment on the back of the AED.

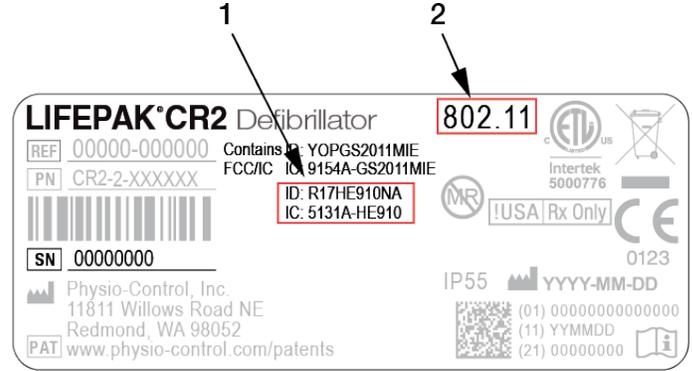

- 1 If this additional pair of ID and IC numbers is present, the AED has cellular capability.
- 2 If this number is present, the AED has Wi-Fi capability.

Check the option that corresponds to your AED.

- USB only (no Wi-Fi or cellular capability)
- Wi-Fi and USB
- Wi-Fi, cellular, and USB

---

# 4

Record the serial number.

Find the AED's serial number as shown below and record it here.

SERIAL NUMBER:

---



---

# 5

Install battery and wait for self-test to complete.

Insert the battery into the battery compartment located on the back of the AED. The device will automatically begin a self-test. This may take up to 2 minutes. Wait until 3 audible tones sound before proceeding to step 6.

**Note:** If the same battery has been previously inserted, the 3 tones will not sound.




---

6

Verify that the Readiness indicator is flashing.

The green Readiness indicator will flash every 6 seconds through a small hole located on top of the lid. A flashing Readiness indicator means the AED is ready for use.

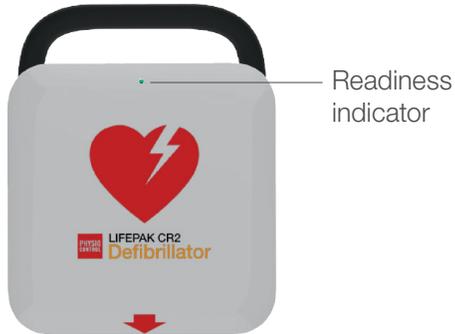

---

7

Check the speaker.

Open the lid and confirm that the voice prompts are audible. Do not respond to the voice prompts at this time. Close the lid to turn off the device.

**IMPORTANT!**

**DO NOT** pull the red handle at this time; only pull in an emergency.



# 8

Refer to Wireless Setup Guide, if applicable.\*

If your AED has wireless capability, please refer to the Wireless Setup Guide included in the box to connect the AED to your LIFELINKcentral AED Program Manager or LIFENET System account. Refer to step 3 in this guide to determine if your AED has wireless capability.

**Note:** LIFELINKcentral AED Program Manager and LIFENET System are not available in all countries.

\*If your AED does not have wireless capability, skip to step 9 in this guide.



---

# 9

## Store the AED and accessories.

Confirm the Readiness indicator is flashing, and place your AED in the location where it will be stored.

If your AED is equipped with a carrying case, place spare electrode trays in the back compartment. Attach the rescue kit to the handle or carrying case strap, if applicable.

Store in a central and accessible location.

- Notify potential users of the location.
- Avoid exposure to moisture or dust.
- Do not store the AED in the presence of flammable gases or in direct contact with flammable material.
- Store at recommended storage temperature: 15° to 35°C (59° to 95°F).



Your **LIFEPAK CR2** Defibrillator  
is now ready for use

---

---

## Training

- **Read the Operating Instructions.**  
The Operating Instructions provide complete directions for use, indications, and potential adverse events. Store the instructions in a convenient location for reference.
- **Watch the training videos.**  
You can find the training videos by visiting the Physio-Control website: [www.physio-control.com](http://www.physio-control.com)
- **Attend formal CPR and AED training.**  
Physio-Control recommends that all identified users attend formal CPR and AED training provided by a recognized training center.

---

## Maintenance

The LIFEPAK CR2 defibrillator conducts daily, weekly, and monthly self-tests to ensure it is ready for use. If your device needs attention and has a wireless connection to your LIFELINKcentral or LIFENET System account, your account administrator will receive an email notification.

If your device does not have a wireless connection, you should check the status at least once a month by confirming that the Readiness indicator still flashes every 6 seconds. If the Readiness indicator does not flash, please refer to the Operating Instructions for troubleshooting information. If you need assistance, call Physio-Control Customer Support or your local authorized distributor. See the contact list included in the box for region-specific phone numbers for Physio-Control.

---

---

## How to get help.

If you need assistance, contact Physio-Control Customer Support. See the contact list included with this guide for region-specific phone numbers. When you call, be prepared to provide your device serial number (recorded in step 4 of this guide).

Physio-Control is now part of Stryker.

---

Physio-Control Headquarters	Customer Support
11811 Willows Road NE	P.O. Box 97006
Redmond, WA 98052	Redmond, WA 98073
<a href="http://www.physio-control.com">www.physio-control.com</a>	Toll Free 800.442.1142
	Fax 800.426.8049

